


Hyperthermia laboratory

Department of Magnetism, IEP SAS, Watsonova 47 , Košice

responsible: M. Molčan, molcan@saske.sk

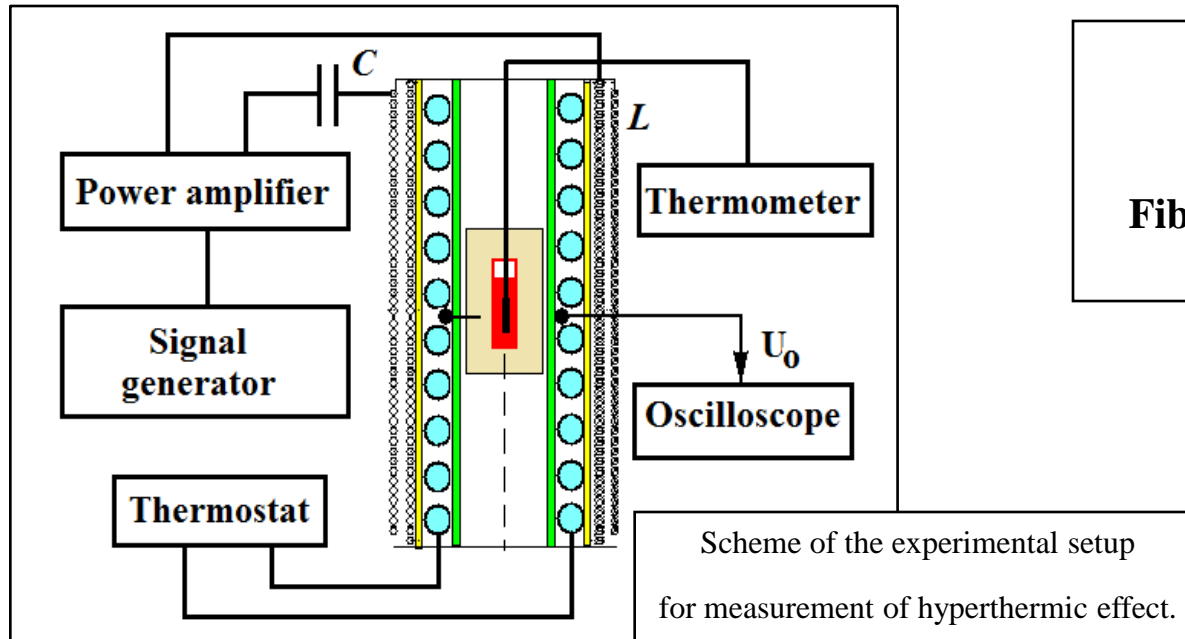

f : 190 – 610 kHz

H : 0 – 8 kA.m⁻¹

Fiber Optic Temperature Sensor
(Accuracy ± 0.1 K)

